


Presto FF-C18

150 x 4.6 mm

HPLC COLUMN APPLICATION

Mucin
ムチン

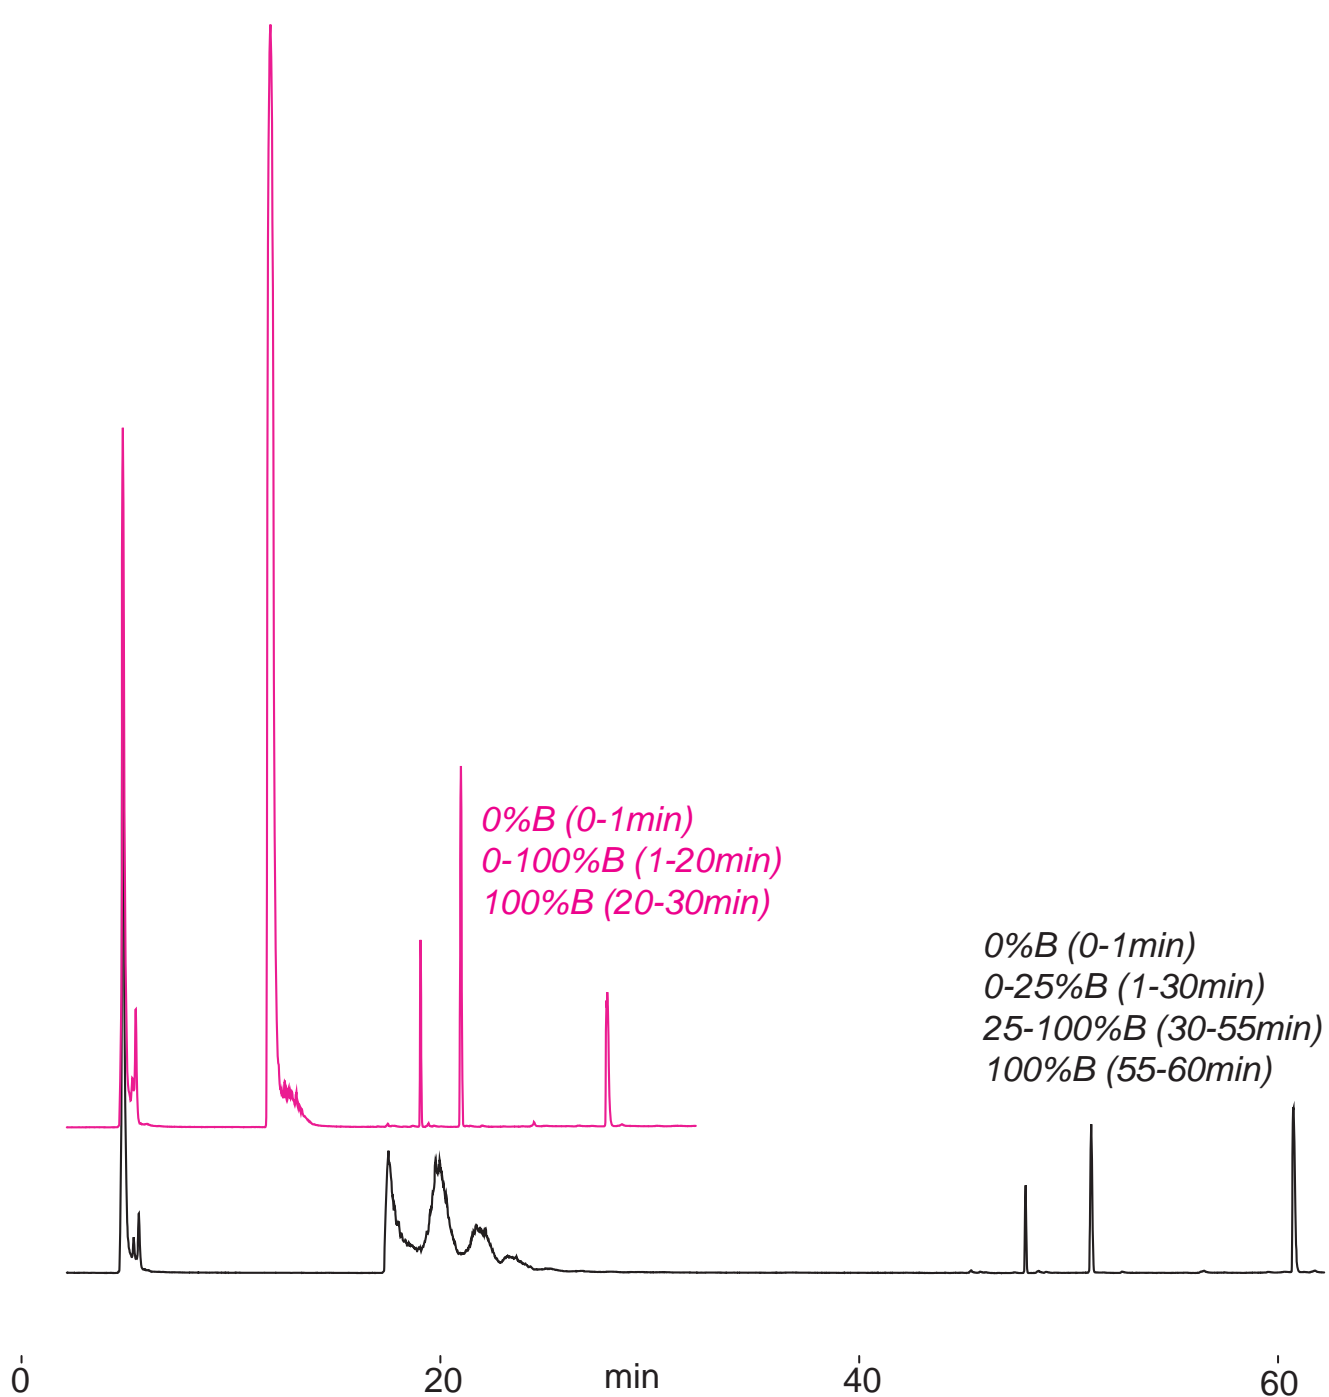

Presto FF-C18, 150 x 4.6 mm
A: 100mM ammonium formate
B: 100mM ammonium formate / acetonitrile = 10 / 90
0.4mL/min (18MPa), 37°C
ELSD (spray chamber 30°C, drift chamber 60°C)
10µL (20mg/mL, 3% ammonia water)