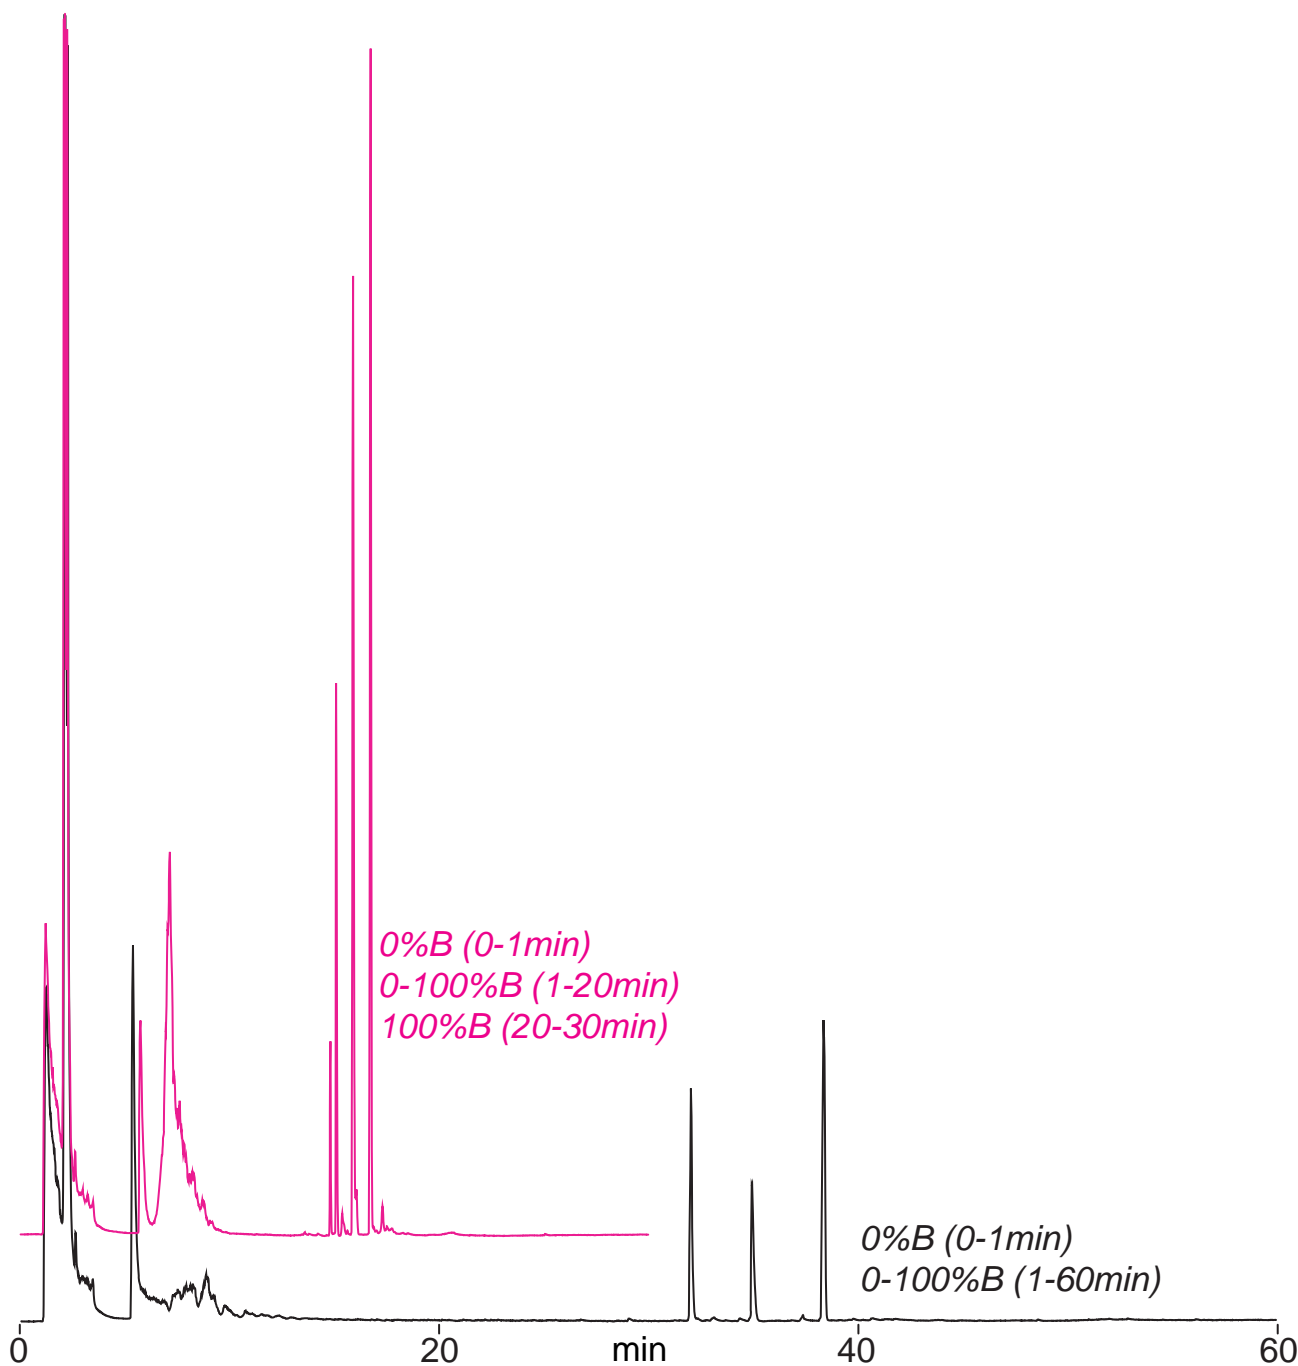


Intrada WP-RP

150 x 4.6 mm

HPLC COLUMN APPLICATION**Mucin**
ムチン

Intrada WP-RP, 150 x 4.6 mm
A: 100mM ammonium formate
B: 100mM ammonium formate / acetonitrile = 10 / 90
1.0mL/min (9MPa), 37°C
ELSD (spray chamber 30°C, drift chamber 60°C)
10µL (20mg/mL, 3% ammonia water)