


Cadenza CD-C18
Unison UK-C18

250 x 4.6 mm


HPLC COLUMN APPLICATION

Isostearic acid


イソステアリン酸



isostearic acid (10mg/mL)

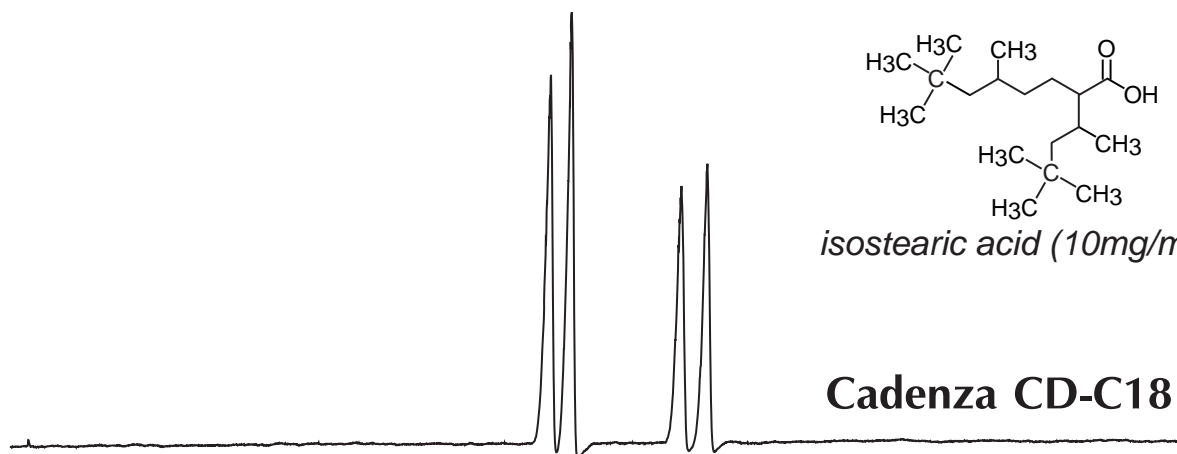

Cadenza CD-C18

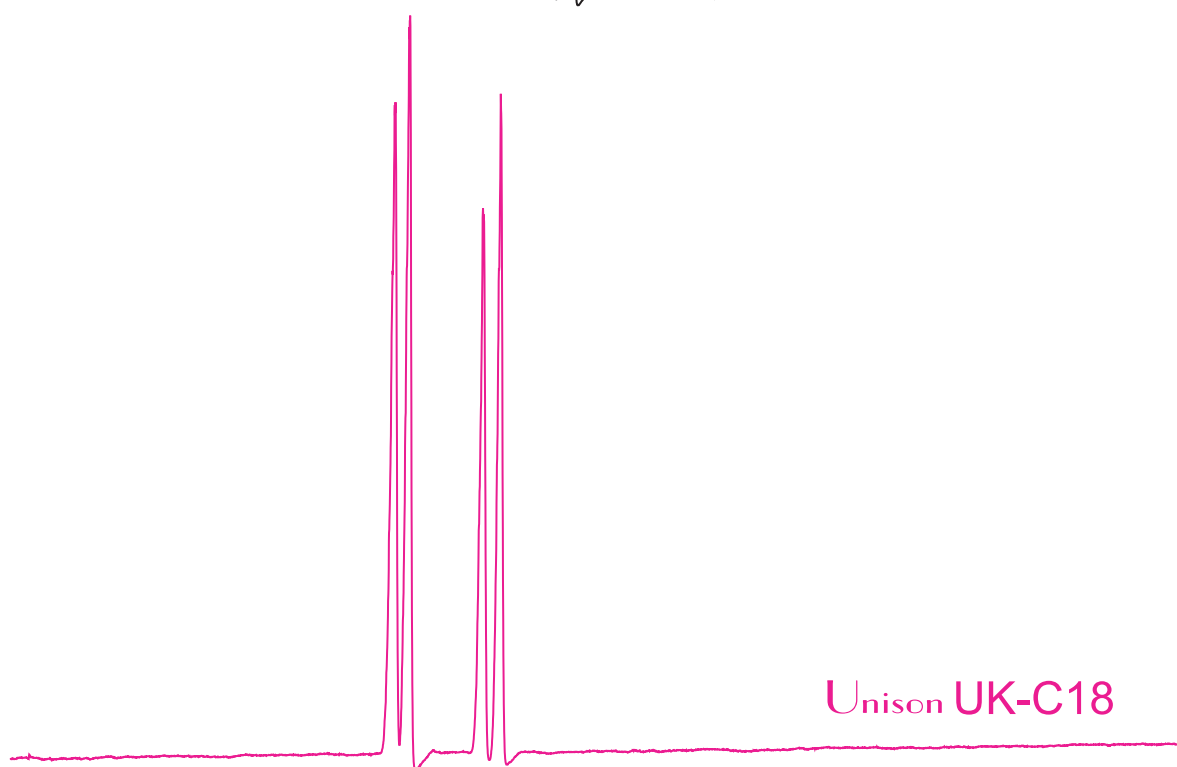

Unison UK-C18

0 60 120 180 min

250 x 4.6 mm

A: 50mM ammonium acetate / acetonitrile = 40 / 60

B: 50mM ammonium acetate / acetonitrile = 38 / 62

0-85%B (0-150min)

1.0mL/min (14MPa), 37°C

ELSD(spray chamber 20°C, drift tube 48C)

20µL (10mg/mL, 100mM ammonium acetate / MeOH = 10 / 90)