


Unison UK-C18
Cadenza CD-C18

250 x 4.6 mm

HPLC COLUMN APPLICATION

Isostearic acid, Stearic acid

イソステアリン酸, ステアリン酸

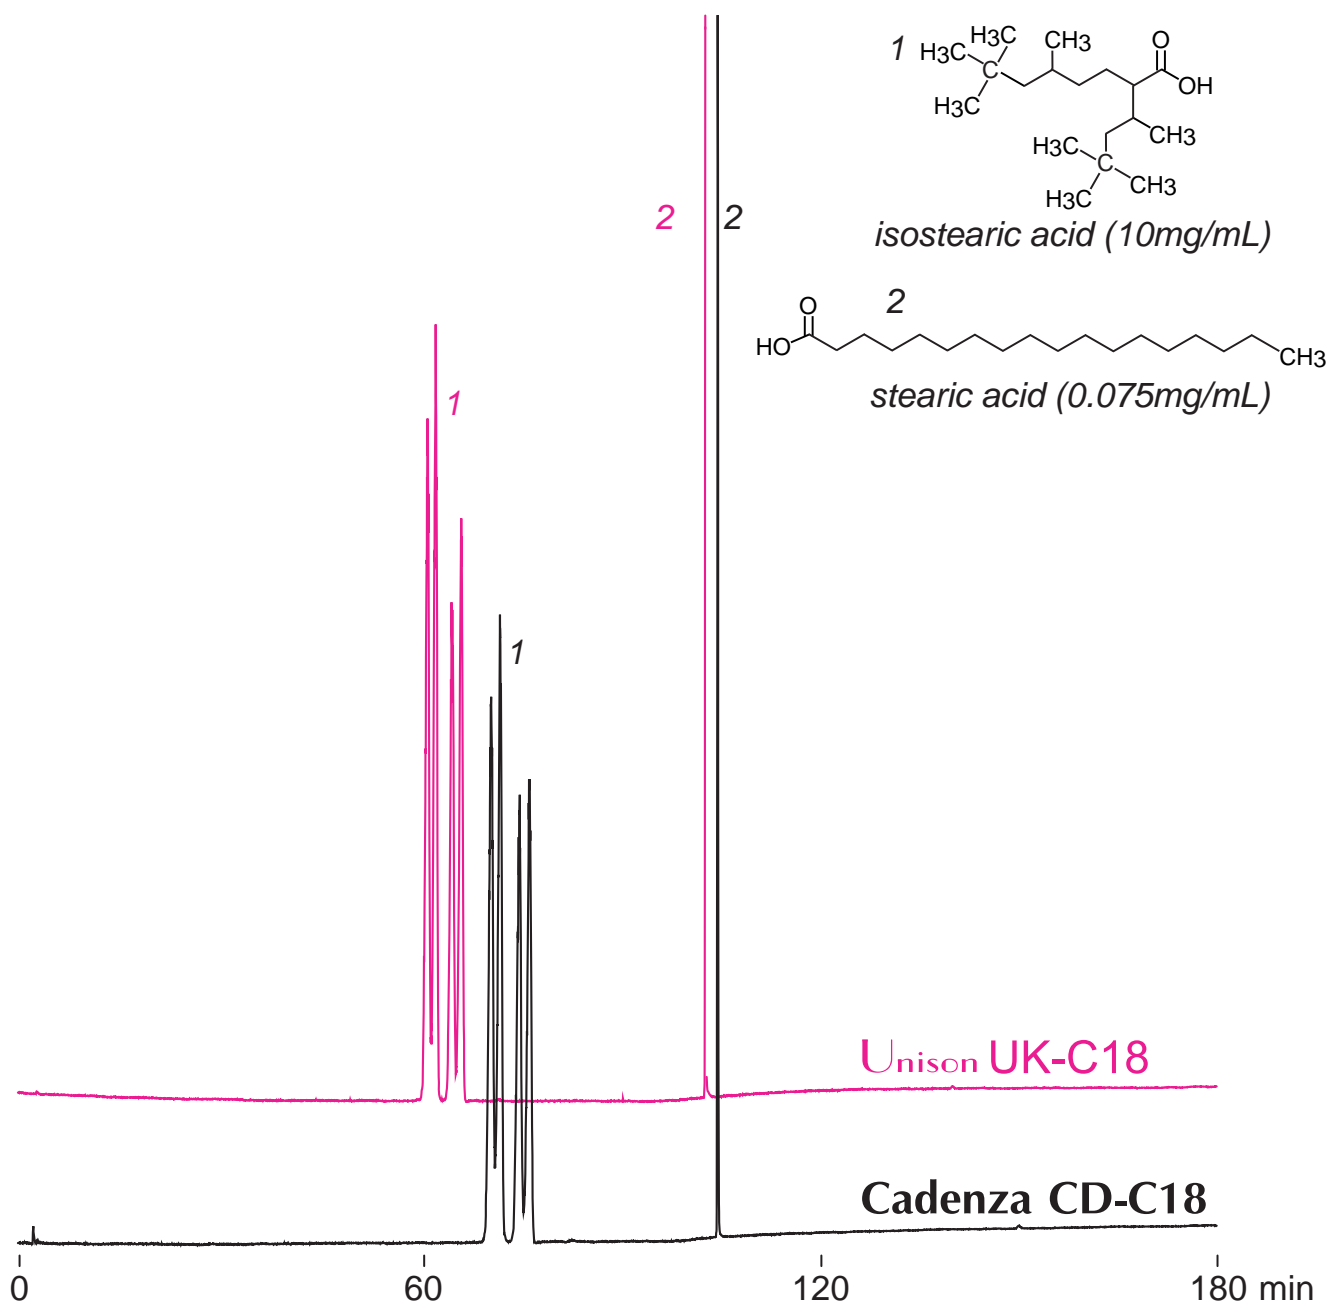

250 x 4.6 mm

A: water / acetonitrile / formic acid = 50 / 50 / 0.1

B: acetonitrile / formic acid = 100 / 0.1

30-40%B (0-90min), 40-100%B (90-100min), 100%B (100-180min)

1.0mL/min (14MPa), 37°C

ELSD (spray chamber 25°C, drift tube 45°C)

20µL (0.075mg/mL, methanol / water / formic acid = 90 / 10 / 1)