


Unison UK-C18
Cadenza CD-C18

250 x 4.6 mm

HPLC COLUMN APPLICATION

Isostearic acid, Stearic acid

イソステアリン酸, ステアリン酸

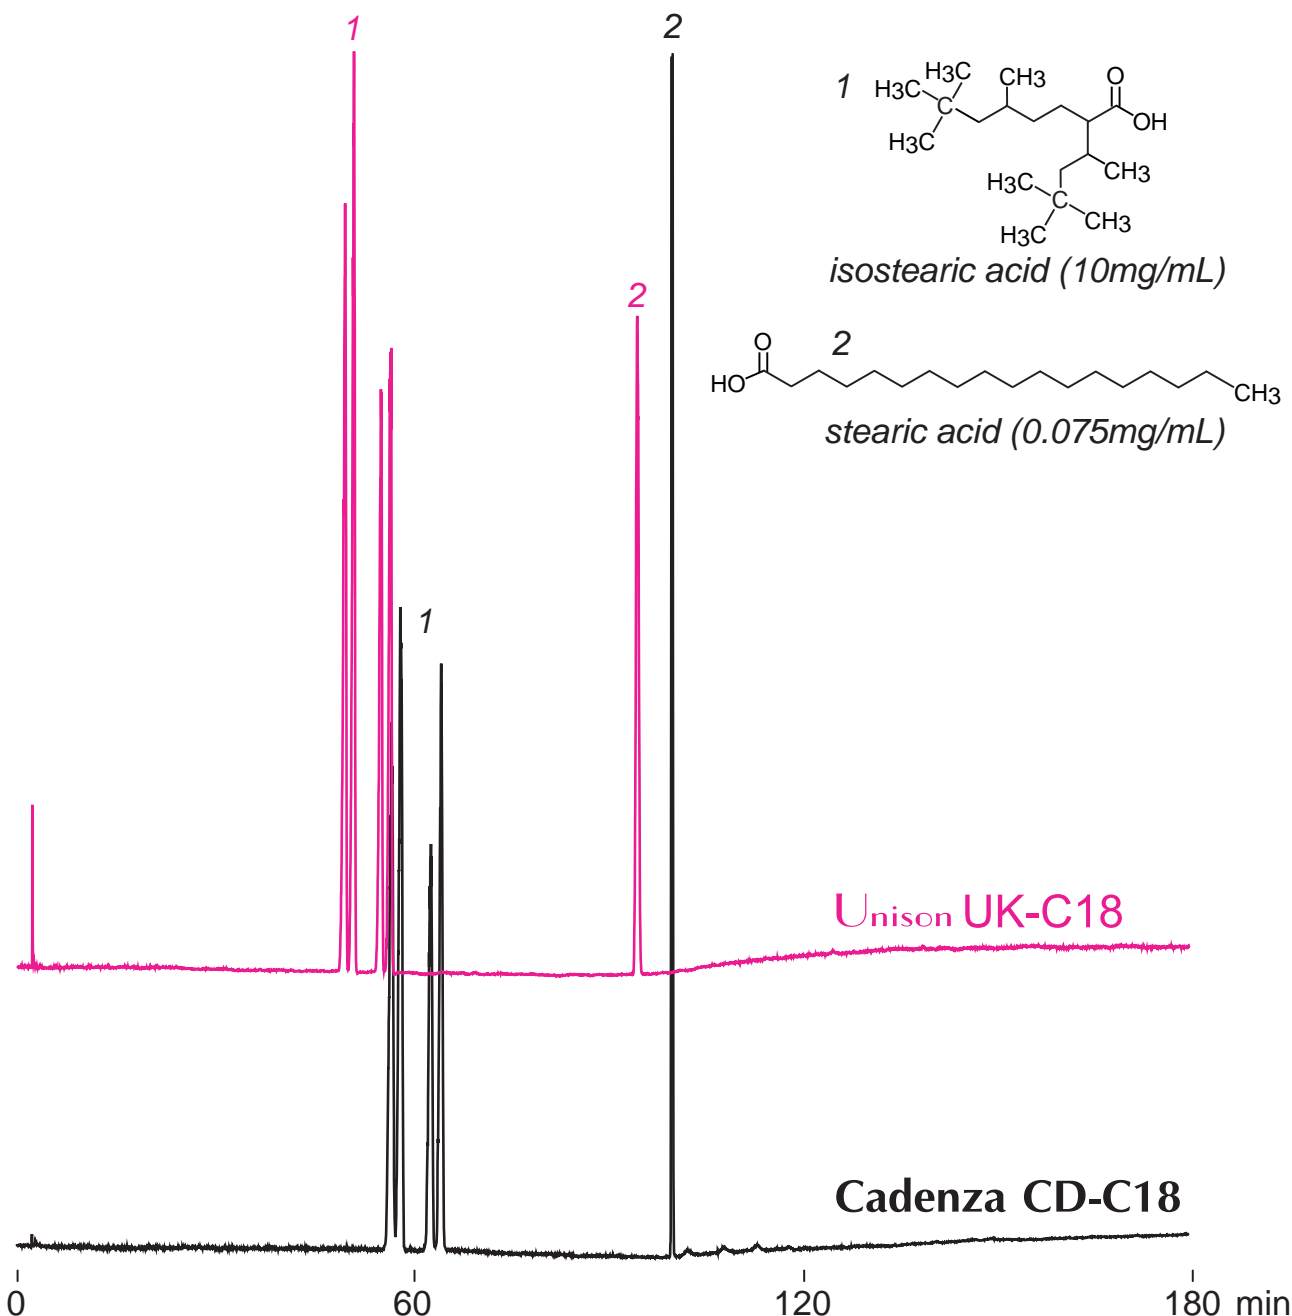

250 x 4.6 mm

A: 100mM ammonium formate / acetonitrile = 50 / 50

B: acetonitrile

30-40%B (0-90min), 40-100%B (90-100min), 100%B (100-180min)

1.0mL/min (14MPa), 37°C

ELSD (spray chamber 20°C, drift tube 48°C)

20µL (0.075-10mg/mL, MeOH / 100mM HCOONH4 = 90 / 10)