

Cadenza CW-C18

Unison UK-C8

Unison UK-Phenyl


Unison UK-C1

100 x 4.6 mm

HPLC COLUMN APPLICATION

Isostearic acid, Stearic acid

イソステアリン酸, ステアリン酸

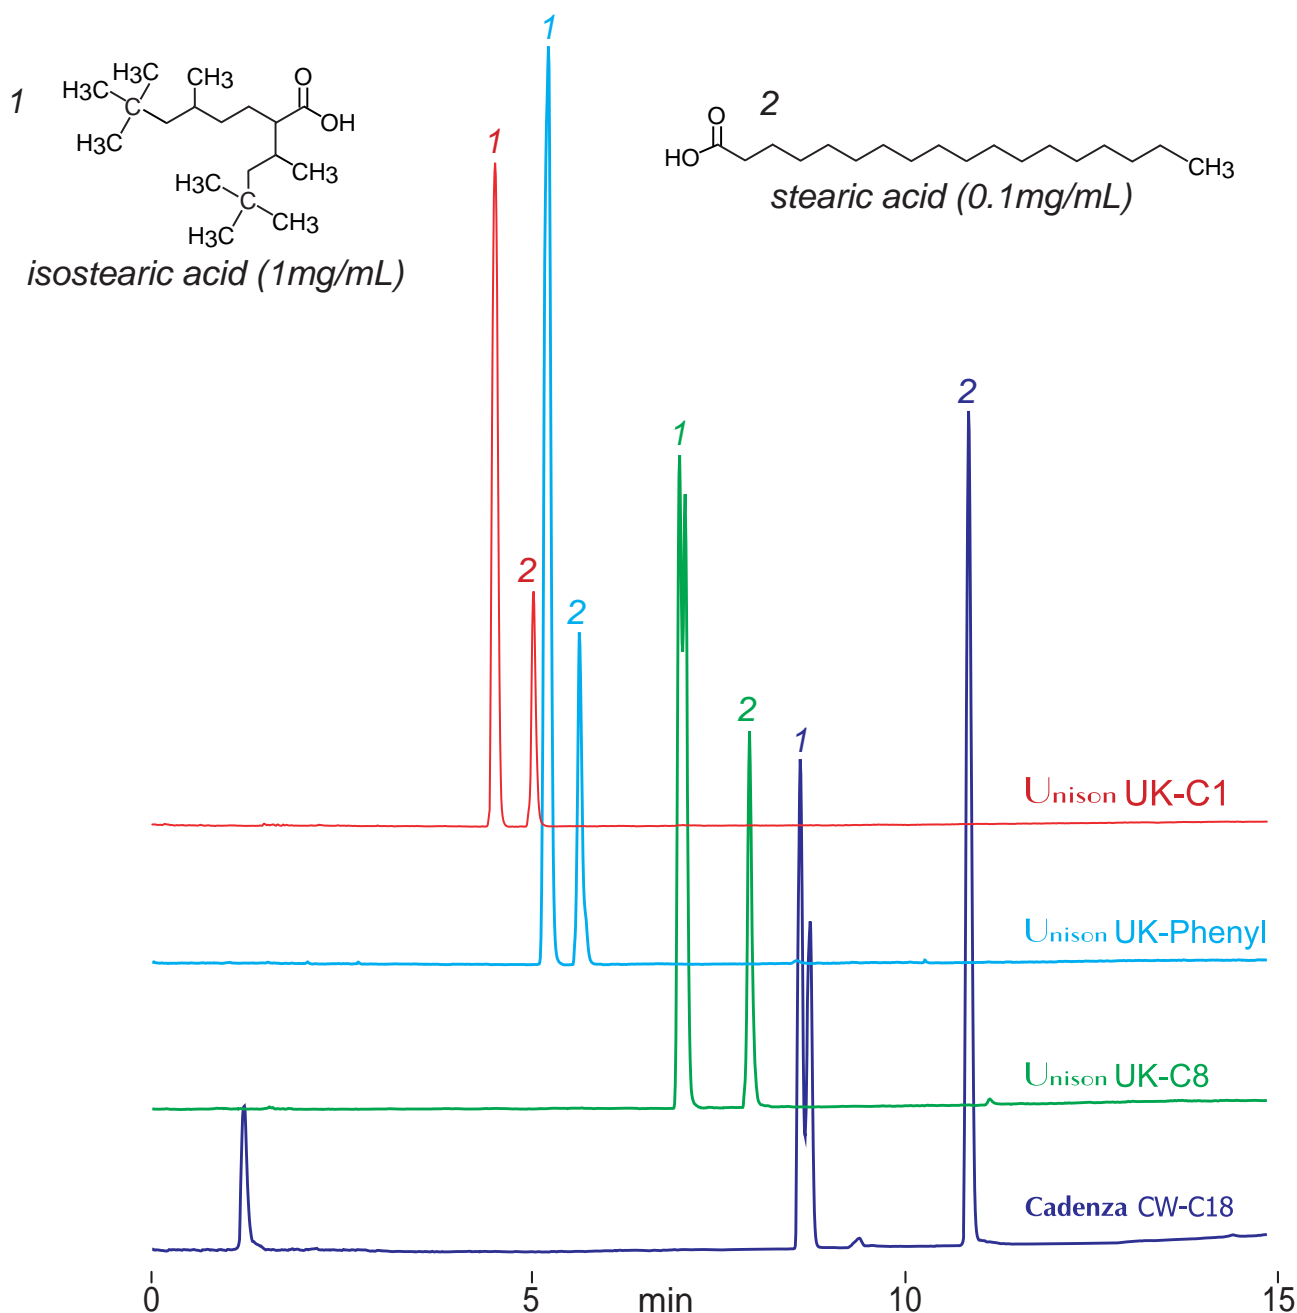

100 x 4.6 mm

A: water / acetonitrile / formic acid = 50 / 50 / 0.1

B: acetonitrile / formic acid = 100 / 0.1

0-100%B (0-10min), 100%B (10-15min)

1.0mL/min (9MPa), 37°C

ELSD (spray chamber 25°C, drift tube 48°C)

10µL (0.1-1mg/mL, MeOH / water / HCOOH = 90 / 10 / 1)