

Unison UK-Phenyl Cadenza CX-C18


Unison UK-C8 Cadenza CW-C18

Unison UK-C18 Cadenza CD-C18 100 x 4.6 mm


HPLC COLUMN APPLICATION

Photoinitiator


光重合開始剤




2-benzyl-2-(dimethylamino)-
4'-morpholinobutyrophenone
0.5mg/mL



diphenyl(2,4,6-trimethylbenzoyl)
phosphine oxide
0.25mg/mL



2,4-diethylthioxanthen-9-one
0.0025mg/mL

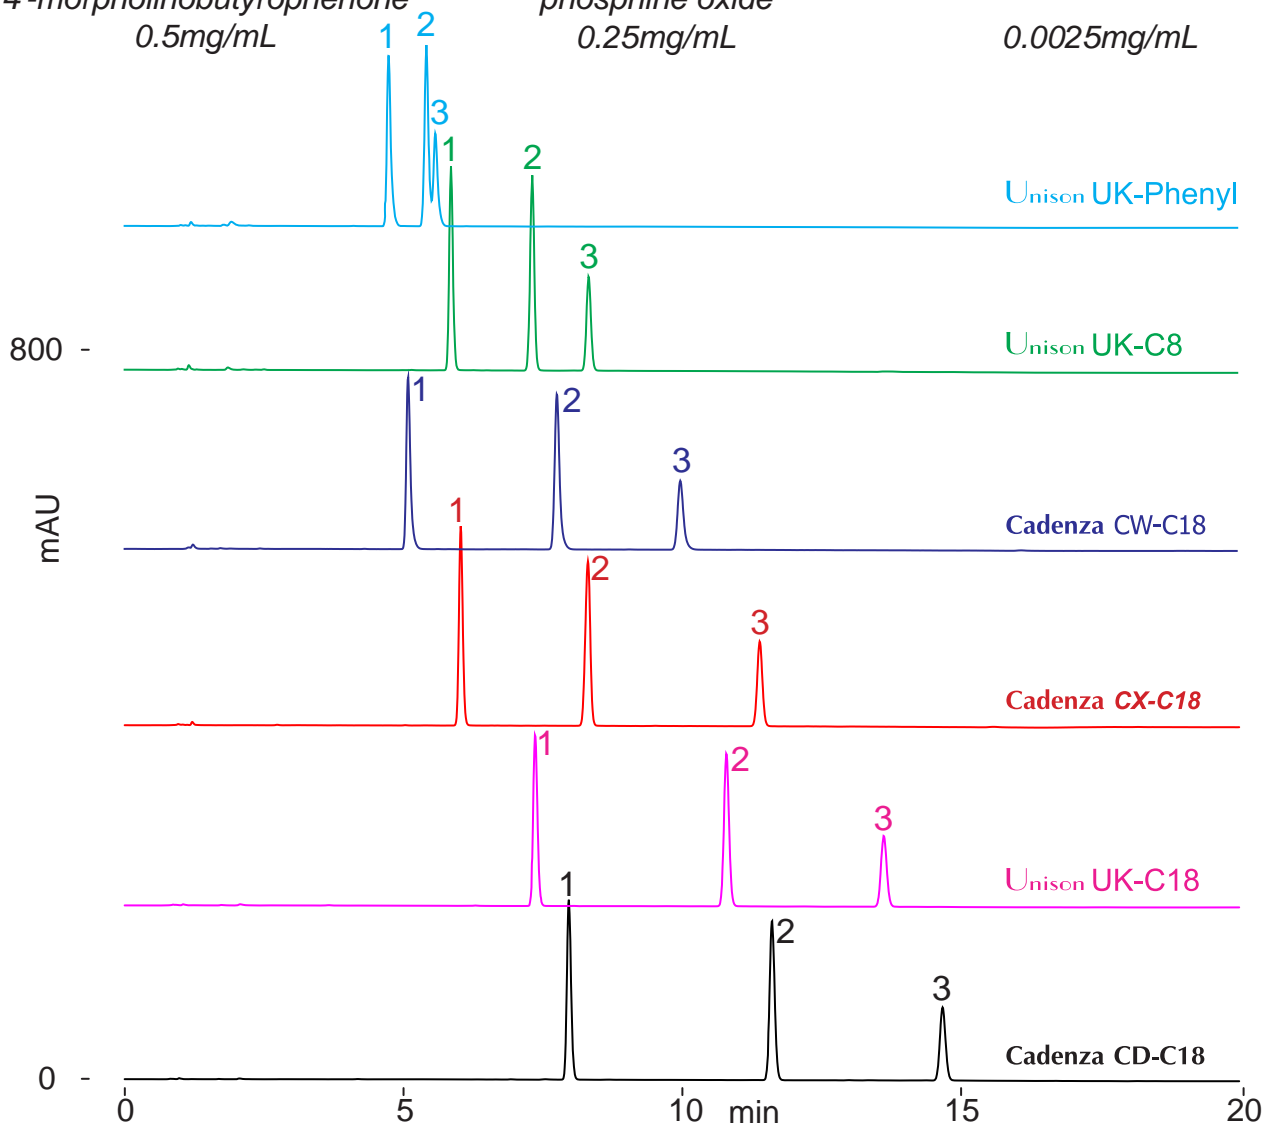

100 x 4.6 mm

A: acetonitrile / 100mM ammonium formate = 50 / 50

B: acetonitrile / 100mM ammonium formate = 90 / 10

0-100%B (0-15min), 100%B (15-20min)

1.0mL/min (9MPa), 37°C, 260nm

10µL (0.0025-0.5mg/mL, acetonitrile / 100mM ammonium formate = 50 / 50)