







Unison UK-C18

100 x 4.6 mm

HPLC COLUMN APPLICATION

Furan derivatives

フラン誘導体

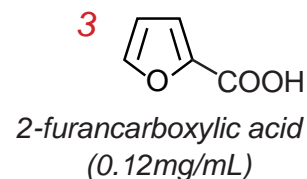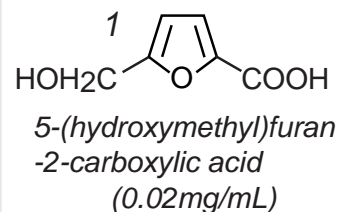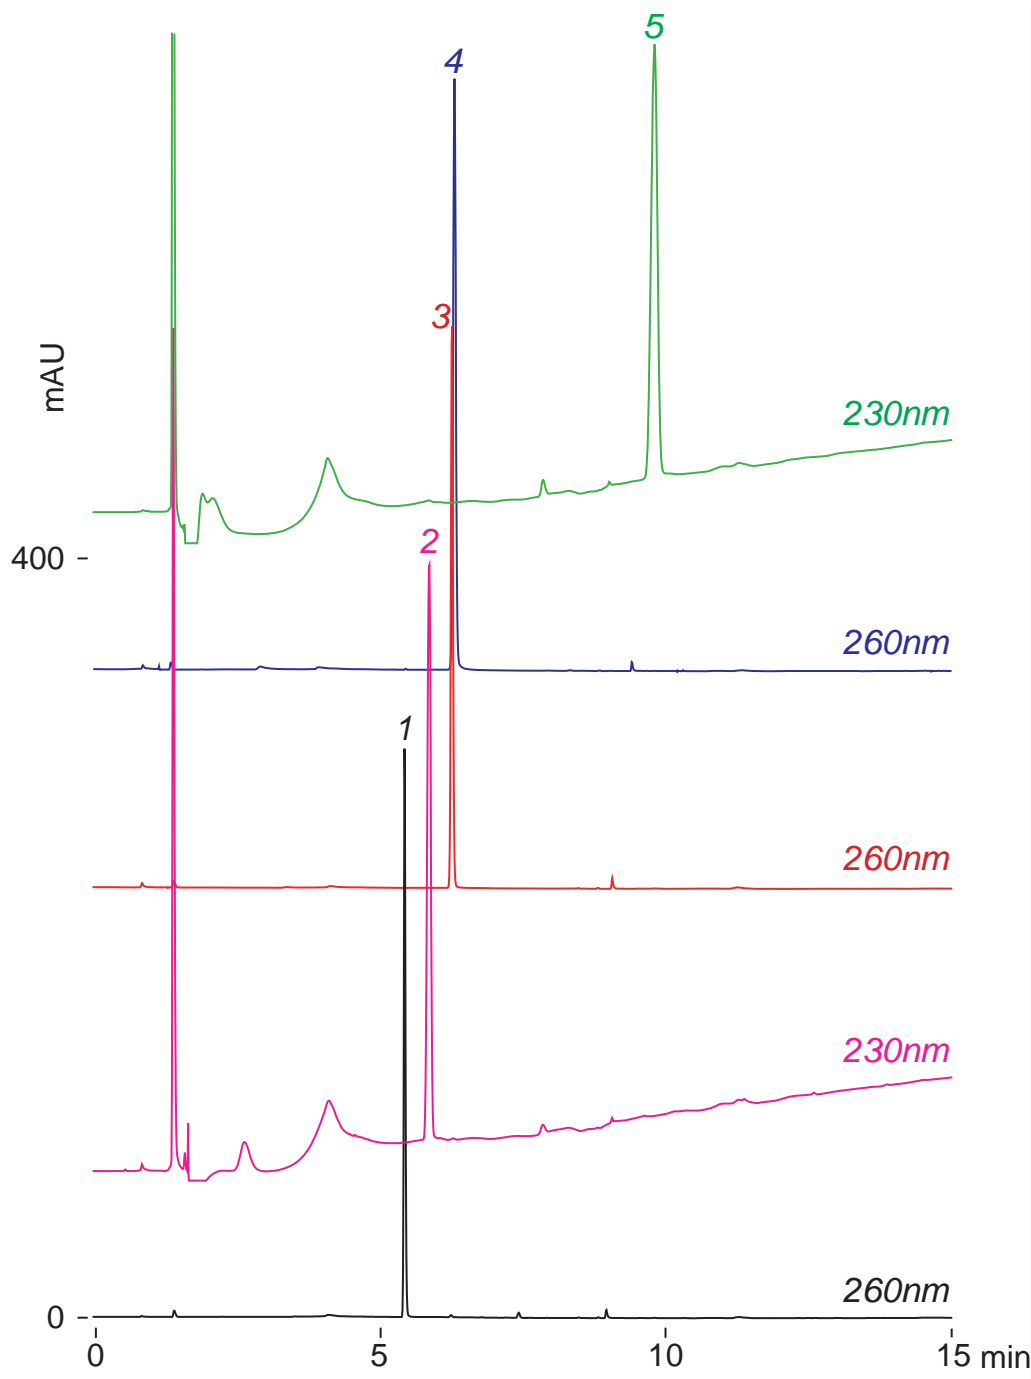

Unison UK-C18, 100 x 4.6 mm
 A: water / formic acid = 100 / 0.1
 B: water / acetonitrile / formic acid = 10 / 90 / 0.1
 0%B (0-1min), 0-75%B (1-15min)
 1.0mL/min (9MPa), 37°C
 10µL (0.02-5mg/mL, water / acetonitrile / formic acid = 50 / 50 / 1)