








Unison UK-C1

250 x 4.6 mm

HPLC COLUMN APPLICATION

## Fatty acid amide

脂肪酸アミドの分析

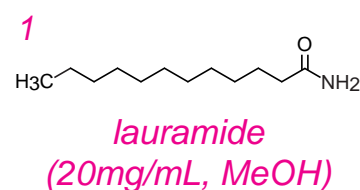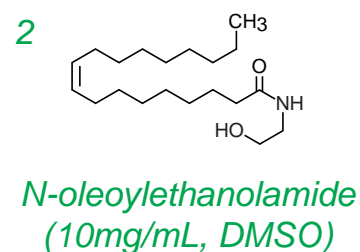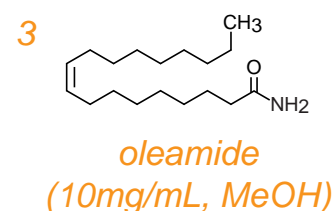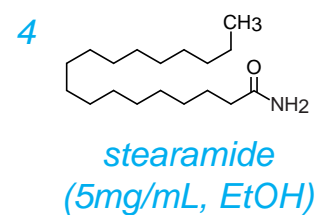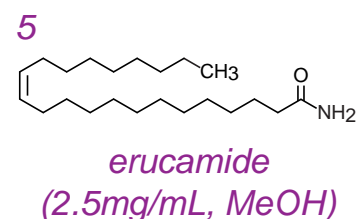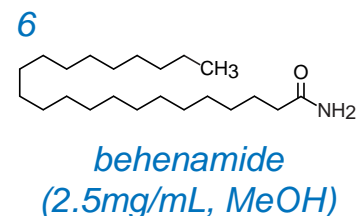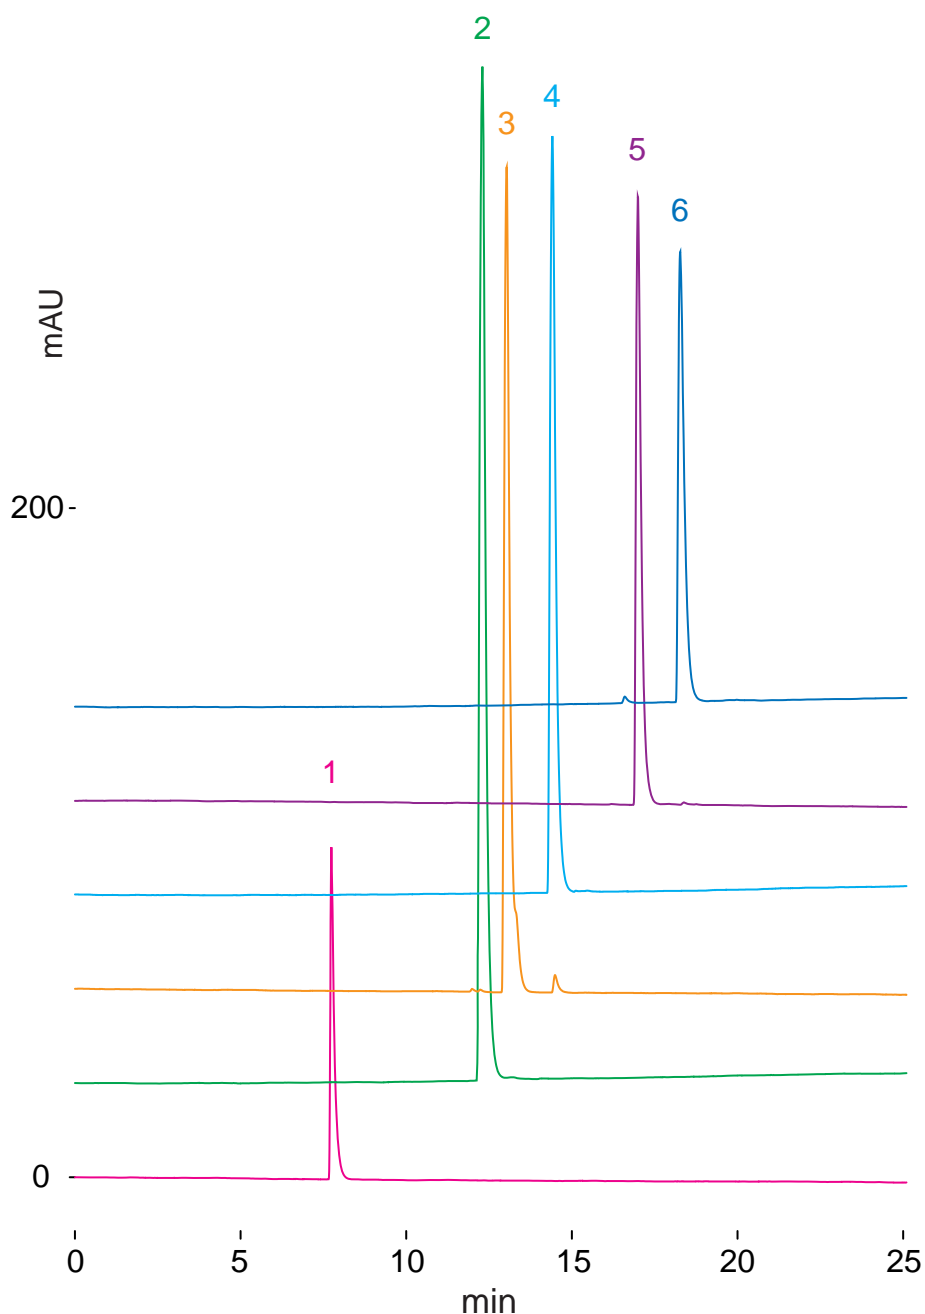

Unison UK-C1, 250 x 4.6 mm

A: water / acetic acid = 100 / 0.5

B: methanol

60 -85%B (0 -20 min), 85%B (20 -25 min)

1.0 mL/min (16MPa), 60°C

ELSD (spray chamber 70°C, drift chamber 100°C)

10 µL (2.5-20mg/mL)