








Unison UK-C8

250 x 4.6 mm

HPLC COLUMN APPLICATION

Fatty acid amide

脂肪酸アミドの分析

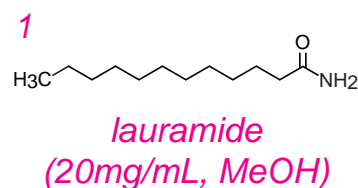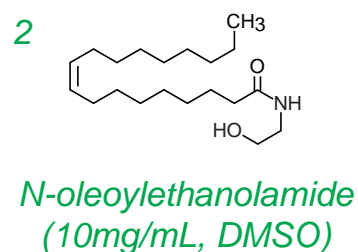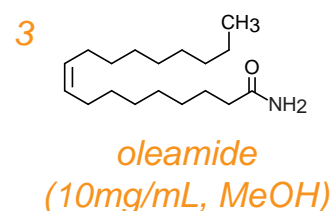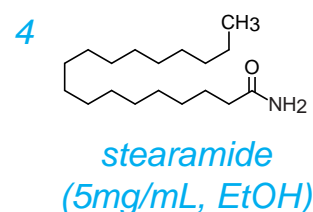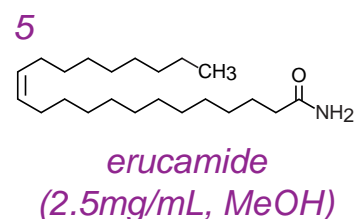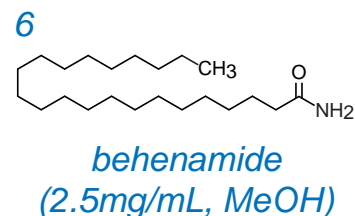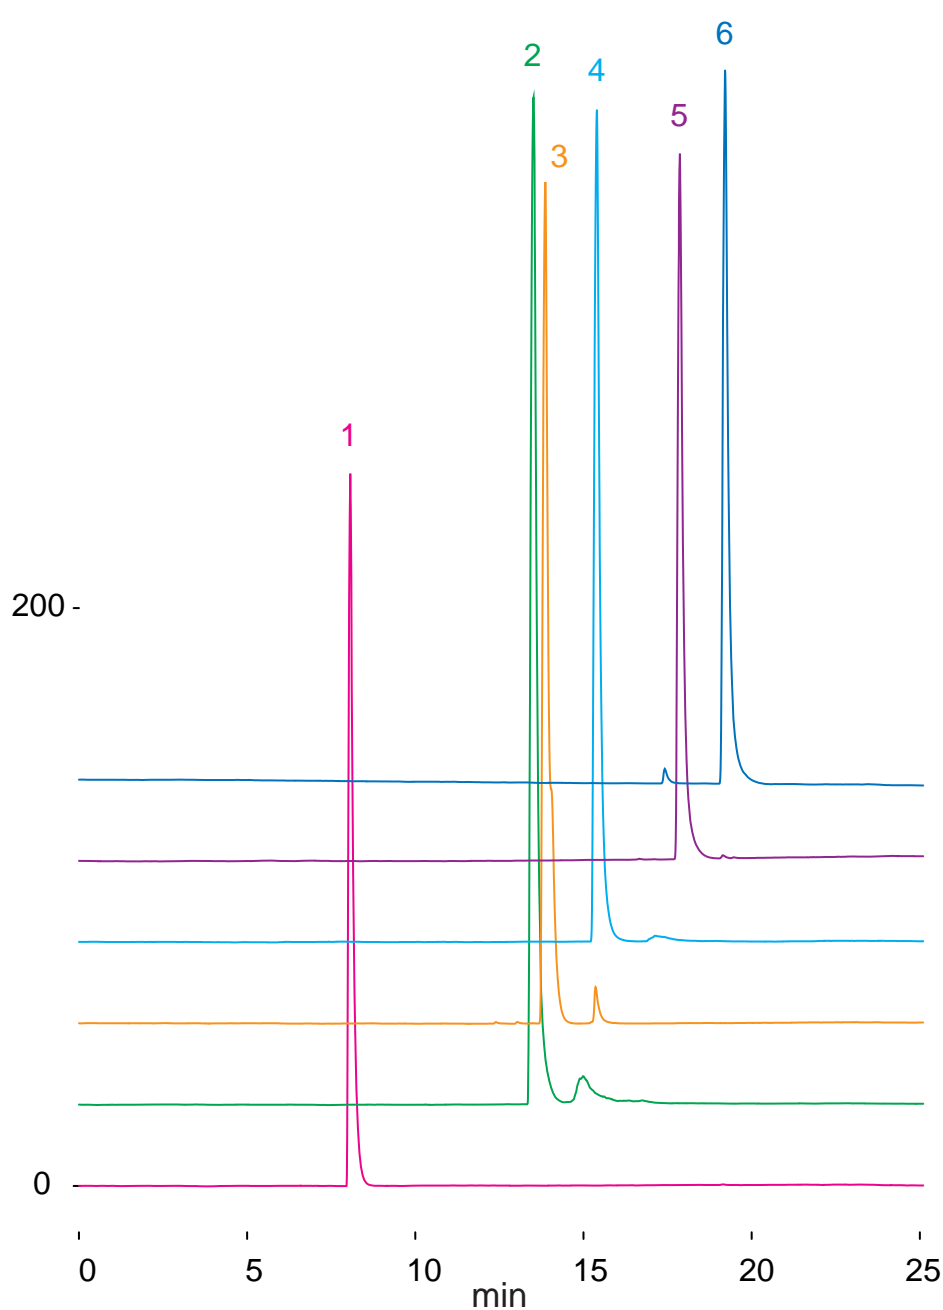

Unison UK-C8, 250 x 4.6 mm  
 A: water / acetic acid = 100 / 0.5  
 B: methanol  
 70 -95%B (0 -20 min), 95%B (20 -25 min)  
 1.0 mL/min (15MPa), 60°C  
 ELSD (spray chamber 70°C, drift chamber 100°C)  
 10 µL (2.5-20mg/mL)