

Unison UK-Phenyl Cadenza CX-C18  
 Unison UK-C8 Cadenza CW-C18  
 Unison UK-C18 Cadenza CD-C18


100 x 4.6 mm

HPLC COLUMN APPLICATION


Organic Redox-Flow Battery negative electrolyte  
 2,2'- (2-Vinylanthracene-9,10-diylidene) bis (1,3-dithiole)

有機レドックスフロー電池負極電解質

9,10-ビス(1,3-ジチオール-2-イリデン)-2-ビニルアントラセン



2,2'- (2-vinylanthracene  
 -9,10-diylidene) bis (1,3-dithiole)

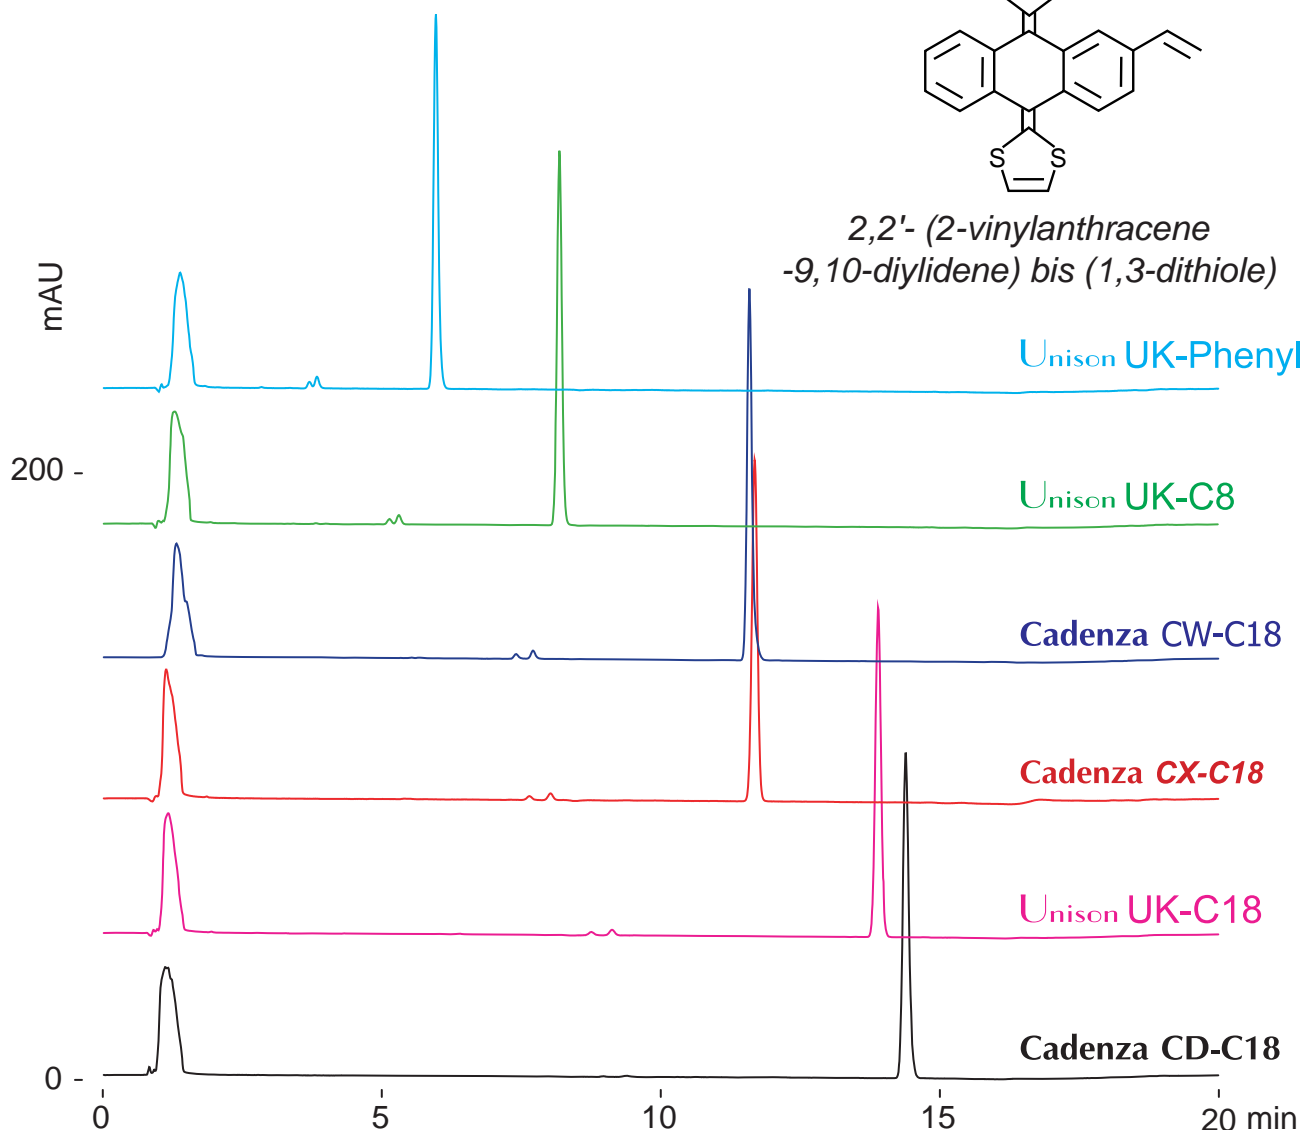

100 x 4.6 mm

A:100mM ammonium formate / acetonitrile = 50 / 15

B:100mM ammonium formate / acetonitrile = 10 / 90

20-100%B (0-20min)

1.0mL/min (9MPa), 37°C, 260nm

10µL (0.05mg/mL, 100mM ammonium formate / DMF = 10 / 90)