


Unison UK-Phenyl Cadenza CW-C18  
 Unison UK-C8 Unison UK-C18  
 Cadenza CX-C18 Cadenza CD-C18 100 x 4.6 mm

HPLC COLUMN APPLICATION

## Donor building block for organic semiconductor ( Halogenated ethylenedioxythiophene analogues)

有機半導体ドナービルディングブロック  
 (ハロゲン化エチレンジオキシチオフエン類縁体)

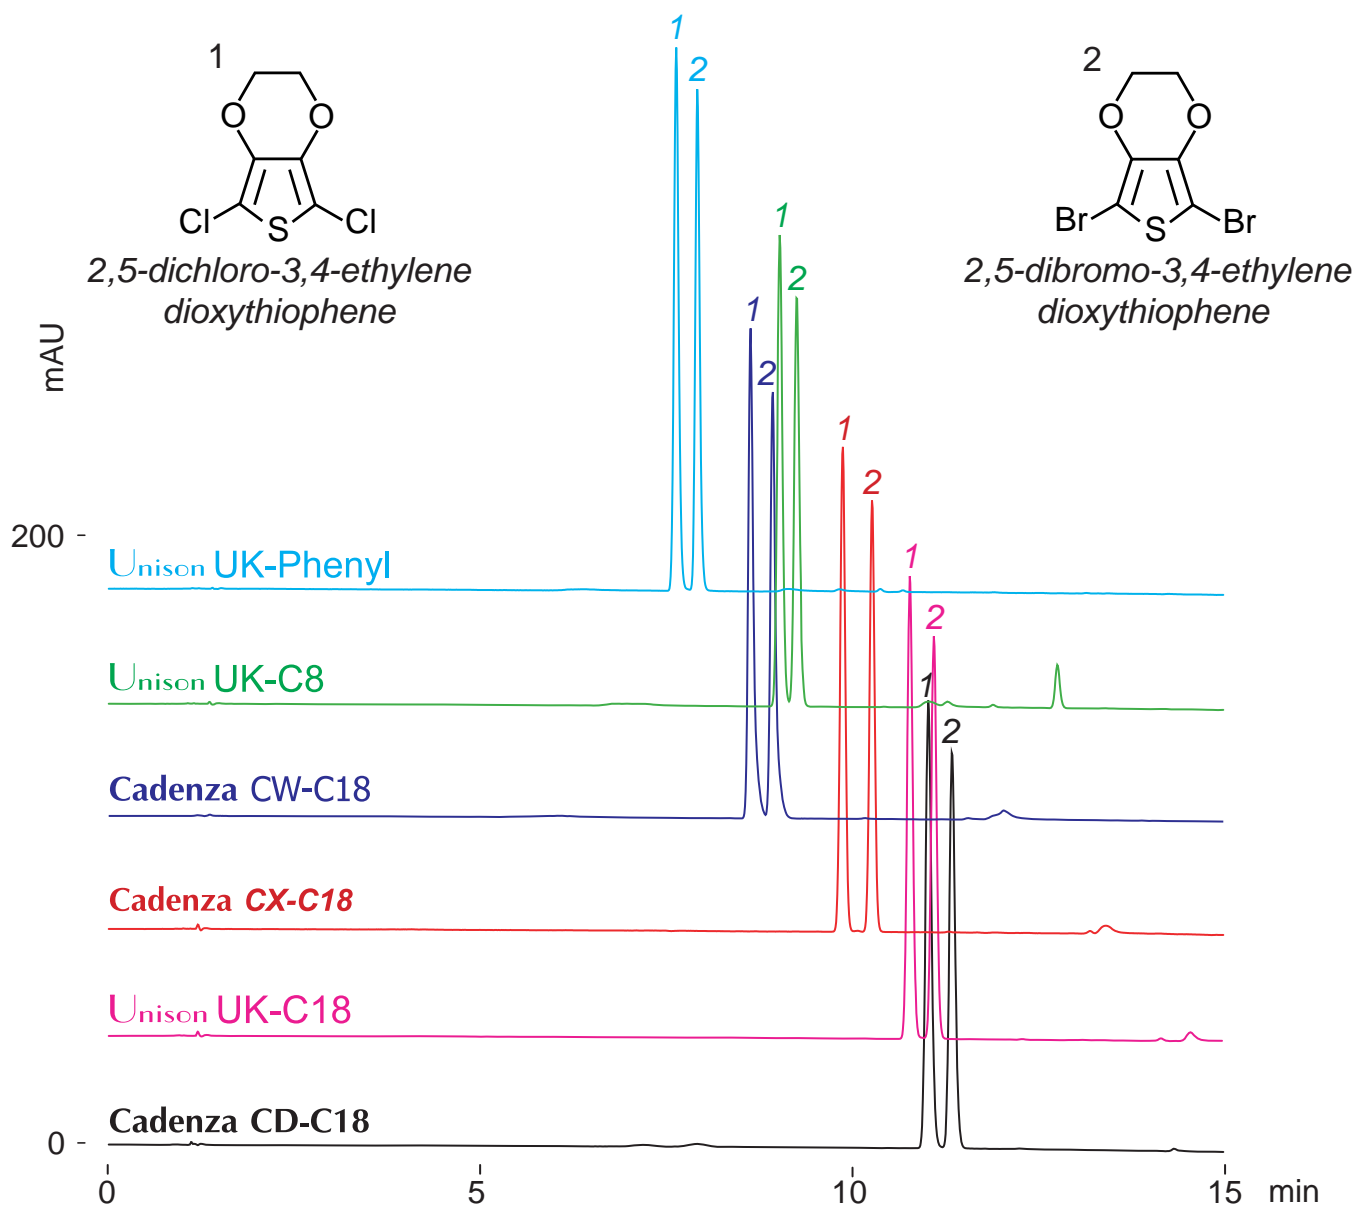

100 x 4.6 mm

A: 100mM ammonium formate / acetonitrile = 90 / 10

B: 100mM ammonium formate / acetonitrile = 10 / 90

20-100%B (0-15min)

1.0mL/min (9MPa), 37°C, 260nm

10µL (0.05mg/mL, 100mM ammonium formate / acetonitrile = 40 / 60)